
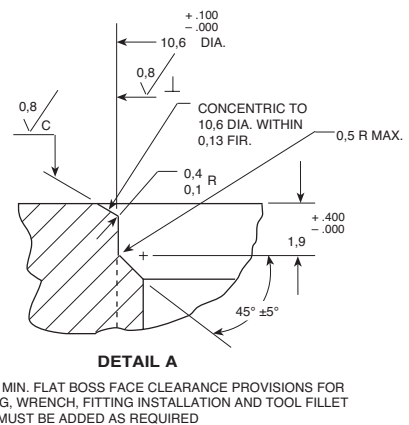
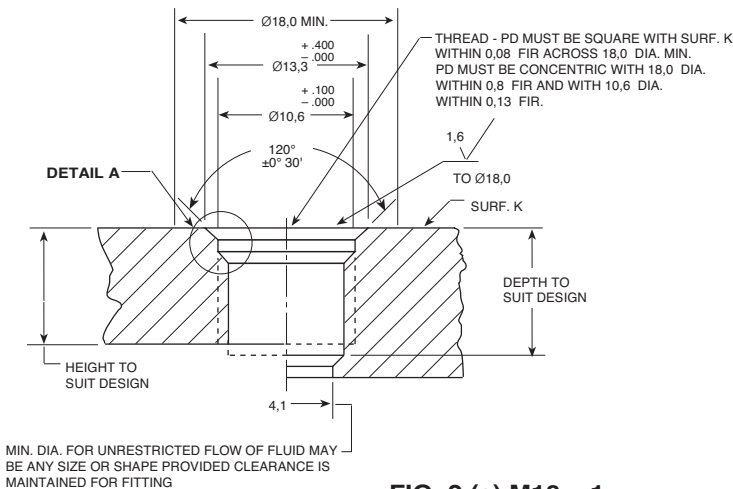
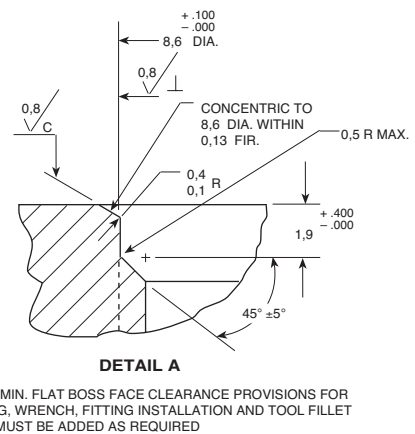
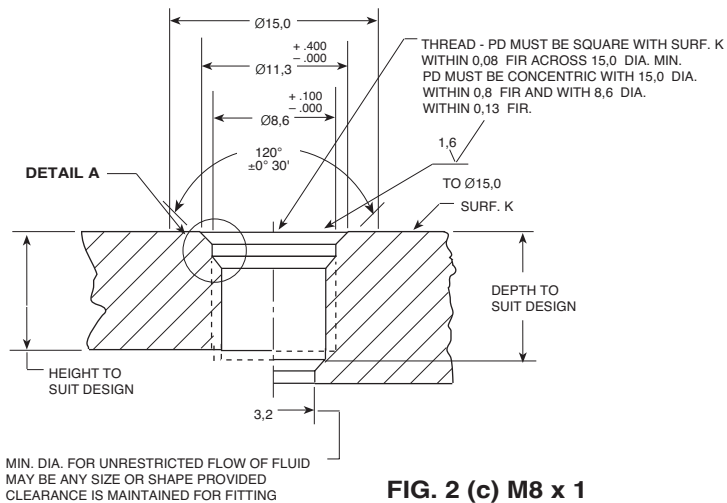
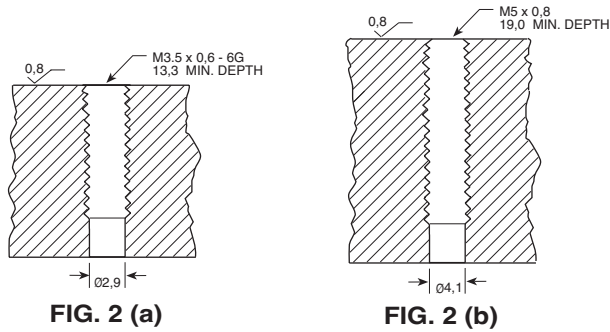


METRIC INSTALLATION OF MINIATURE THREADED SERIES TRANSDUCERS

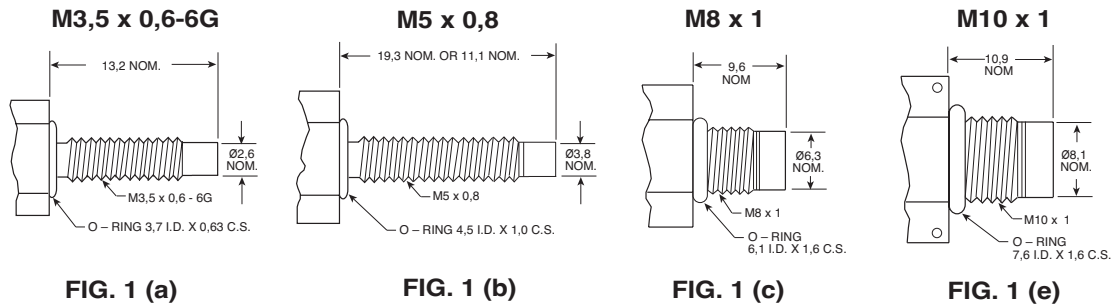

For proper mounting of Figures 1(e), an ISO7320 port is required. The detail for this port is shown in Fig. 2 (e) and Fig. 2 (e) Detail. Mounting torque for the transducers is listed below.



M3,5 x 0,6-6G	M5 x 0,8	M6 x 1-6g	M8 x 1	HKS-375M ONLY	M10 x 1	M10 x 1
1,7 Nm (Max.)	1,7 Nm (Max.)	6 Nm (Max.)	8,5Nm (Max.)		20,3 Nm	9-13,5 Nm

(Q)



METRIC INSTALLATION OF MINIATURE THREADED SERIES TRANSDUCERS

CRYOGENIC SERIES



CTL-190M
M5X0,8

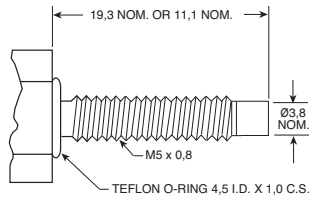



CTL-312M
M8X1

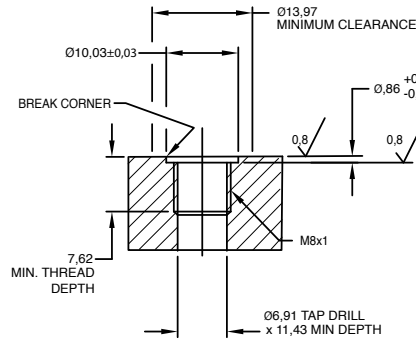



CTL-375M
M10X1

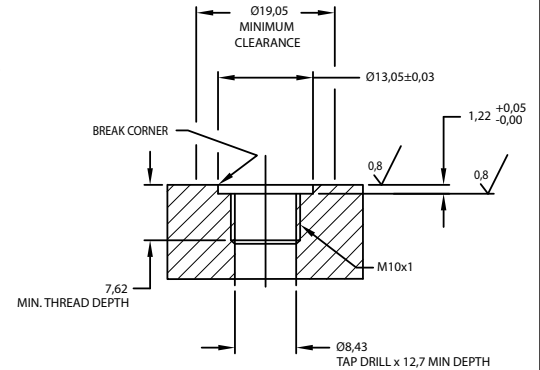



(E)WCT(V)-312(M)

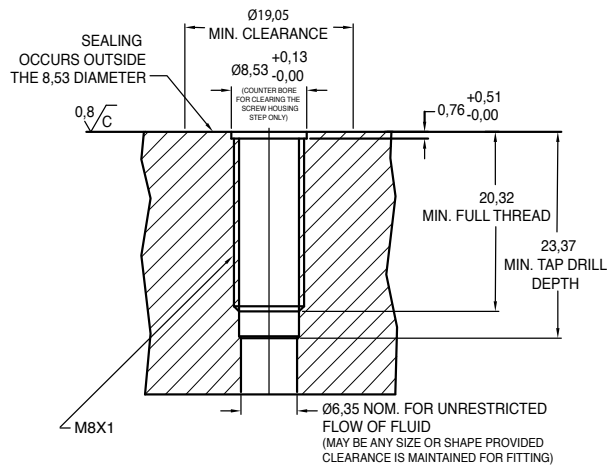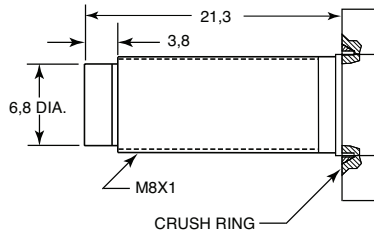

ETL-GTS-X-312(M)
MAKS - 8/8T




TTS-X-235(M)

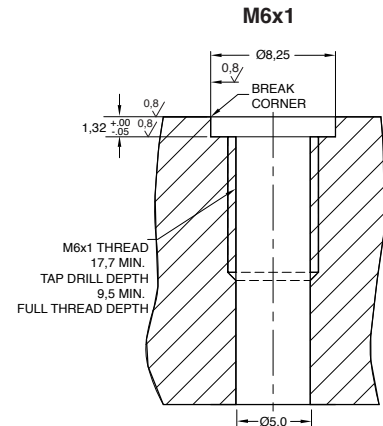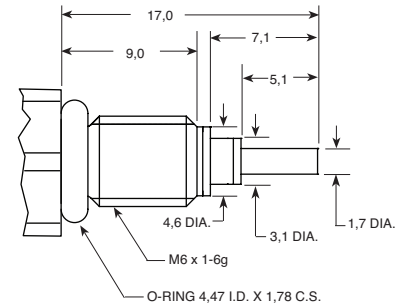


(Q)

METRIC INSTALLATION OF MINIATURE THREADED SERIES TRANSDUCERS

KZS SERIES

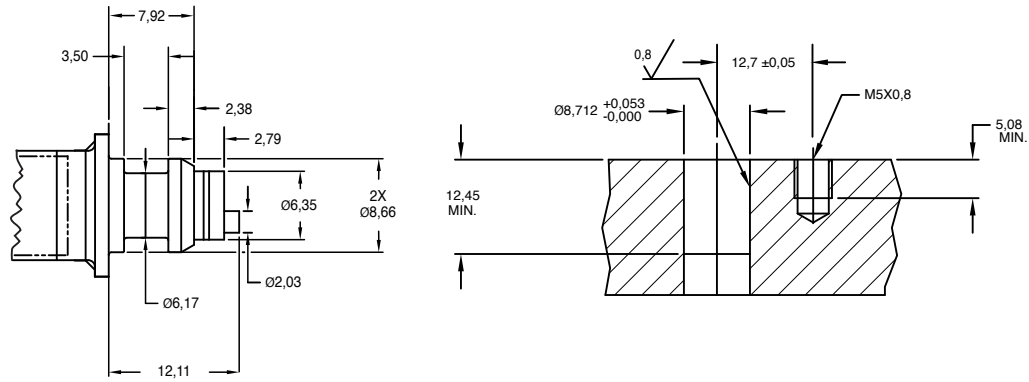

MAKS-6(X)

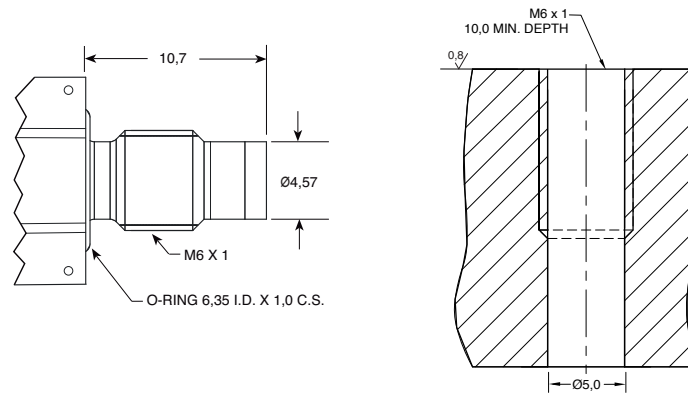

HKL-1-235M HKL/T-1-235M

